



innovation in
geotechnical
instrumentation

Calibration Record

RST Instruments Ltd., 11545 Kingston St., Maple Ridge, British Columbia, Canada V2X 0Z5
Tel: 604 540 1100 • Fax: 604 540 1005 • Toll Free: 1 800 665 5599 (North America only)
e-mail: info@rstinstruments.com • Website: www.rstinstruments.com

Vibrating Wire Pressure Transducer

Customer : PT Unggul Ejawantah Industri
Model : VW-2100A-1.0
Serial Number : VW37174
Mfg Number : 337090
Range : 1000.0 kPa
Temperature : 20.0 deg C
Barometric Pressure : 1012.0 millibars
Cable Length : 145 meters
Cable Colour Code : red/black (coil) Green/white (thermistor)
Cable Insulation / Jacket : PEPolyethylene / PVC 6EL380004
Thermistor Type : 3 kΩ

Applied Pressure (kPa)	Readings Up (B units)	Readings Down (B units)	Average Readings (B units)	Calculated Linear (kPa)	Linearity F.S. Error (%)	Polynomial Fit (% FS)
0.0	9891	9891	9891	2.3	0.22	0.01
208.0	9126	9126	9126	207.5	-0.05	-0.01
418.0	8355	8355	8355	414.1	-0.19	-0.02
624.0	7578	7578	7578	622.3	-0.16	0.01
832.0	6798	6798	6798	831.7	-0.03	0.02
1040.0	6013	6013	6013	1042.1	0.20	-0.01
Max. Error (%)					0.22	0.02

Linear Calibration Factor :

Regression Zero :

Temperature Correction Factor :

C.F. = 0.26815 kPa / B unit
At Calibration Bi = 9899.3 B unit
Tk = -0.19794 kPa / deg C rise

Polynomial gage Factors A : -1.0950E-06 B : -0.25073 C : 2587.1

Pressure is calculated with the following equations :

Linear, $P \text{ (kPa)} = C.F. \times (Li - Lc) - [Tk(Ti - Tc)] + [0.014504 (Bi - Bc)]$

Polynomial, $P \text{ (kPa)} = A(Lc)^2 + BLc + C + Tk(Tc - Ti) - [0.014504(Bc - Bi)]$

	DATE	VW2104	TEMP degC	BARO
	(dd/mm/yy)	Pos.B (Li)	(Ti)	(Bi)
SHIPPED ZERO READINGS :	13-Dec-18	9889	22.2	1016.4

Li, Lc = initial (at installation) and current readings

Ti, Tc = initial (at installation) and current temperature deg C


Bi, Bc = initial (at installation) and current barometric pressure readings, in millibars

B units = B scale output of VW 2102, VW 2104 readouts

B units = Hz2/1000 ie. 1700Hz = 2890 B units

Certified By : I. Kurchavov *IK*

Date : 13-Dec-18

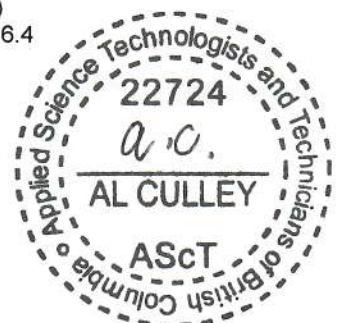

This instrument has been calibrated using standard traceable to the NIST in compliance with ANSI Z540-1